


# Modified Clinical Test of Sensory Interaction on Balance - mCTSIB

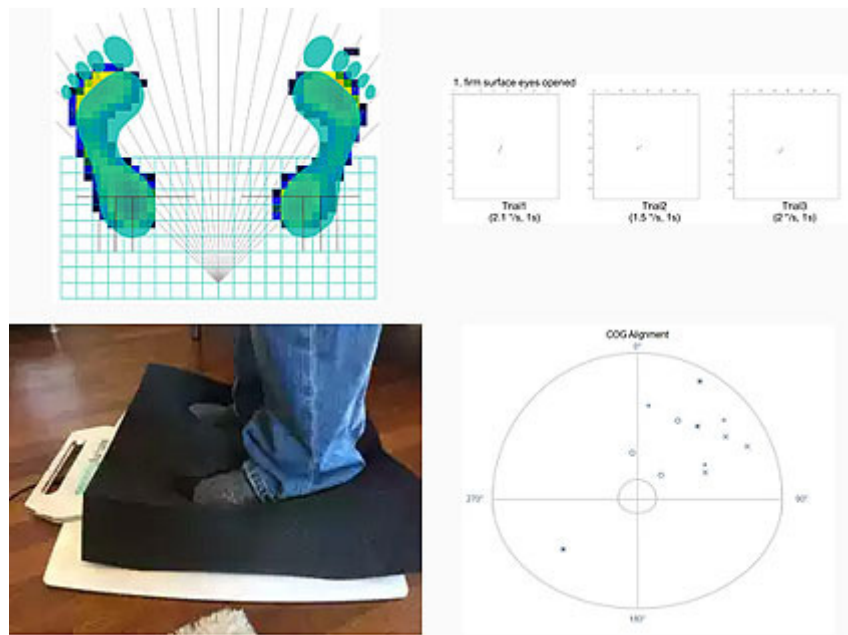

mCTSIB protocol allows the measurement of static balance in four sensorial conditions:

- 1- Stable surface and open eyes;
- 2- Stable surface and closed eyes;
- 3- Surface instable and eyes open;
- 4- Surface instable and eyes closed.

Outputs with normative values comparison: Sway velocity; mean sway velocity, composite sway velocity; CoP alignment